

USER MANUAL



EXOQUICK® ULTRAPURE EV ISOLATION KIT FOR SERUM AND PLASMA

Store Kits at +4°C - +30°C upon receipt

Cat # EQ UltraPure

A limited-use label license covers this product. By use of this product, you accept the terms and conditions outlined in the License and Warranty Statement contained in this user manual.



System
Biosciences

Version 1
9/24/2025

FUELING YOUR INNOVATION

CONTENTS

Product Description	2-3
Kit Contents	3
Protocol	4-5
Example Data and Applications	6-8
Technical Support	9
Licensing and Warranty Statement	9-10



PRODUCT DESCRIPTION

Why choose between yield and purity?

With **SBI's ExoQuick® UltraPure**, you get both. This next-generation hybrid EV isolation kit combines gentle precipitation with advanced spin-column technology to deliver **maximum yields of pure, apoB-free, intact EVs in just 20 minutes** - no ultracentrifuge required. Compared to size-exclusion chromatography (SEC) and other polymer-based methods, ExoQuick® UltraPure (or EQ UltraPure) achieves **lower albumin carry-over and higher purity**, making it the smarter choice for reliable EV isolation.

- **Dual-Action Innovation** – integrates SBI's proprietary ExoQuick® gentle precipitation with advanced mixed-mode affinity spin columns for unmatched purity and yield
- **Small Sample Compatibility** – efficient EV isolation from as little as 100 µL to 250 µL of serum or plasma
- **ExoQuick® UltraPure: Unmatched Quality, Backed by Data** - the only kit delivering high yield, high purity, concentrated EVs with superior protein, total RNA, and cleaner samples

ExoQuick® UltraPure vs. SEC and Ultracentrifugation

Key Metric	EQ-UltraPure	SEC (company Q)	Ultracentrifugation (UC)	Key Takeaway
Yield (particles / mL serum or plasma)	(1.5×10^{12}); High Consistency	(5.7×10^{10}); Highly varied	(4.2×10^8); Lowest recovery	Best in class; Great for any downstream applications
Purity (particles / mg protein)	(3.0×10^{11})	(1.8×10^{11})	(1.2×10^{11})	Good for in-vitro/in-vivo studies, cargo loading for therapeutics; functional assays
EV Particle Concentration per Prep. (particles / mL)	(8.2×10^{11}) 30× higher than SEC method; 120× higher than UC	(2.8×10^{10}); Highly inconsistent	(6.8×10^9)	Most Convenient (Save time and frustration)
EV Protein Yield (µg / mL serum or plasma)	(4887)	(310)	(3.5); Lowest	Best for Downstream Analysis (Proteomics, Biomarker Discovery, Functional Assays)
Total RNA (ng / mL serum or plasma)	(18-20 ng)	n/a	n/a	Based on BioAnalyzer; Great for RNA-Seq.
Lipoprotein Removal	> 90% apoB depletion	~ 20 % apoB dep.	~ 15% apoB dep.	Cleaner Sample (less contaminants to worry)

The ExoQuick® UltraPure workflow can be completed in as little as 1 hour with less than 20 minutes of hands-on time.

Simply add ExoQuick solution to serum or plasma samples (free of cellular debris), centrifuge to collect the EV pellet, resuspend, and apply directly to the EQ UltraPure purification column. Incubate, then spin to collect EVs in the flow-through.

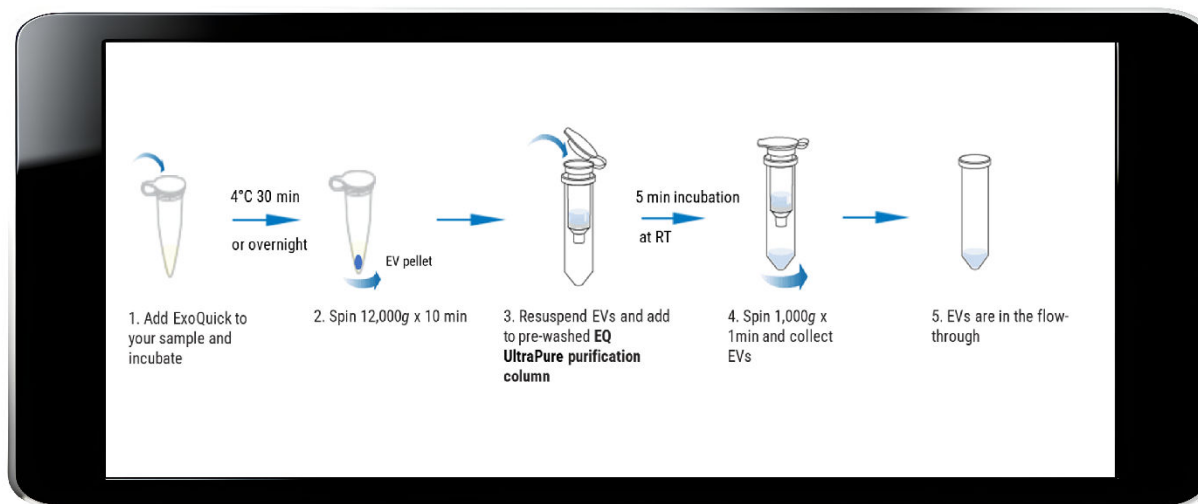


FIGURE 1. EXOQUICK® ULTRAPURE WORKFLOW

KIT CONTENTS

Component	Volume / Qty	Storage Temperature
ExoQuick®	1 mL, Sterile	+4°C to +30°C
UltraPure Purification Column	10 columns	
Column Buffer	25 mL	
Collection Tubes	10	
2 mL Eppendorf Tubes	10	

***1 reaction is defined as 250ul of serum/plasma precipitated using ExoQuick.**

The kit is shipped at +4°C to +30°C and should be stored at +4°C - +30°C. Properly stored kits are stable for 6 months from the date received.

Component not included in the kit: Sterile 1xPBS

PROTOCOL

GENERAL INFORMATION

NOTE: For plasma samples, the addition of thrombin (Cat #TMEXO-1) to generate a serum-like fraction is an optional step - especially for sensitive applications such as mass spectrometry, where added proteins may interfere with the detection of low-abundance targets.

A. ExoQuick Precipitation

1. Collect the biofluid and centrifuge it at $3,000 \times g$ at room temperature for 15 minutes to remove cellular debris.

2. Transfer the supernatant to a new tube.

! **OPTIONAL:** If additional debris remains detectable, centrifuge the supernatant for an additional 10 minutes at $12,000 \times g$ then transfer the supernatant to a new tube.

3. Add the appropriate volume of ExoQuick to the clarified biofluid, as shown in the table.

Biofluid	Sample Volume	ExoQuick Volume	Incubation Time
Serum/plasma	250 ul	63 ul	30 min or O/N at 4°C

4. Mix thoroughly by inverting or shaking the tube, then incubate at 4°C for 30 minutes or overnight. Rotation during incubation is not required.

NOTE: To achieve a higher yield of EVs, overnight incubation at 4°C is recommended.

5. Centrifuge the ExoQuick/biofluid mixture at $12,000 \times g$ for 10 minutes. Centrifugation can be performed at either room temperature or 4°C with comparable results. After centrifugation, EVs may appear as a beige or white pellet at the bottom of the tube.

6. Carefully aspirate the supernatant. If residual fluid remains, centrifuge briefly and remove all traces by aspiration, taking care not to disturb the EV pellet.

7. The EV pellet may be sticky; please resuspend it gently and patiently in 500 μ L of sterile 1 $\times$ PBS.

B. Purification of Isolated EVs

1. Take the **UltraPure purification column** (containing resin in storage buffer) and remove both the cap and the bottom closure.
2. Place the column into an empty **collection tube** and loosely screw the cap onto the top of the column.
3. Centrifuge at $1000 \times g$ for 1 min to remove the storage buffer.

4. Discard the flow-through and return the column to the collection tube.
5. To wash the column, remove the cap and apply 500 µl of **Column buffer** onto the resin. Loosely screw the cap back onto the top of the column.
6. Centrifuge at 1,000 x g for 1 min. Discard the flow-through.
7. Repeat the wash step once more.
8. Discard the collection tube.
9. The column is now ready for sample application.
10. Insert the stopper to plug the bottom of the column.
11. Add the entire EV sample from step A-7 to the resin. Secure the screw cap **tightly** on top of the column.
12. Mix EV sample thoroughly with the resin by inverting and flicking the column at room temperature (RT). Then place the column on a rotating shaker for 5-7minutes.

C. Sample Elution

1. Prepare a **2ml Eppendorf tube** to collect the EV sample.
2. Remove the bottom closure, immediately place the column into the **2ml Eppendorf tube**, and loosen the cap halfway.

! CAUTION: Once the bottom closure is removed, the sample will begin to flow out of the column. We strongly recommend keeping the cap loosely inserted, as residual liquid may still be present in the cap.
3. Centrifuge at 1000 x g for 1 min to collect the EVs.
4. Store the isolated EVs:
 - a) **For immediate use:** Store at +4°C for up to one week
 - b) **For long-term storage:** Store at -20°C or -80°C

Please Note: To preserve structural and functional integrity, we recommend adding 1/10 volume of [EV-Guard™ EV Storage Buffer – 10X concentrated \(EXSBA-10\)](#) for long term storage.

EXAMPLE DATA AND APPLICATIONS

ExoQuick® UltraPure delivers superior EV purity with higher yields

Western blot of serum-derived EVs shows EQ UltraPure retains key EV markers (CD9, CD81, TSG101) while reducing albumin contamination compared to ExoQuick®, ExoQuick® Ultra, and SmartSEC™ Single (Figure 2).

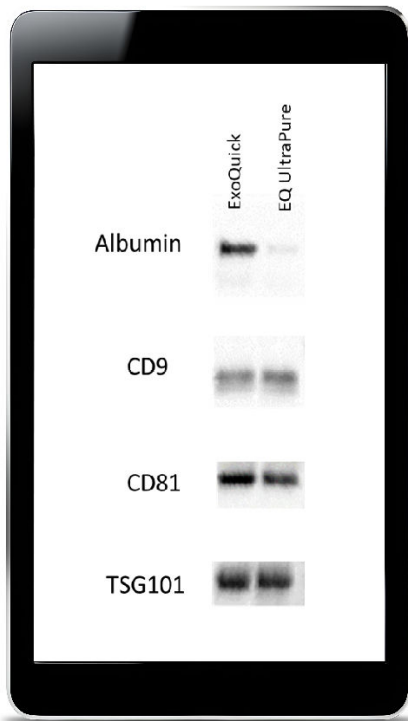


FIGURE 2. EXOQUICK® ULTRAPURE DELIVERS HIGHER YIELDS OF PURE EVS.

ExoQuick® UltraPure Sets a New Benchmark in EV Isolation Performance

EVs were isolated from serum using EQ UltraPure, SEC, and ultracentrifugation. EQ UltraPure shows the strongest EV marker signals (CD9, TSG101), the lowest albumin contamination, and delivers the highest EV yields by protein and fNTA compared to SEC and ultracentrifugation (Figure 3).

(A) Western blot analysis. Each lane was loaded with an equal amount of EV protein. **(B)** Total EV protein yield per mL of serum. EV protein concentration was measured using a NanoDrop spectrophotometer.

(C) Fluorescent nanoparticle tracking analysis (fNTA) demonstrates the superior EV yields obtained with EQ UltraPure compared to SEC and ultracentrifugation.

(D–E) Comparative analysis of EV isolation methods based on yield per input serum volume (D, per mL) and per input EV protein (E, per mg).

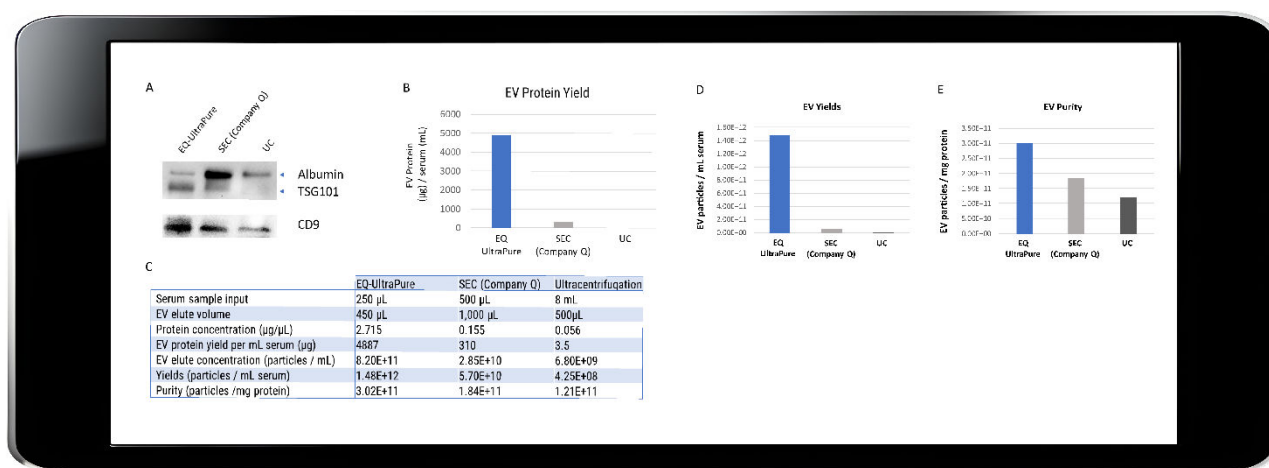


FIGURE 3. EXOQUICK® ULTRAPURE OUTPERFORMS TRADITIONAL EV ISOLATION METHODS

ExoQuick® UltraPure = Cleaner Intact EVs, Fewer Lipoproteins

ELISA analysis shows EQ UltraPure removes ~96% of ApoB from serum, yielding the lowest lipoprotein contamination. In contrast, SEC and ultracentrifugation preparations contain 3–4× higher ApoB levels (Figure 4).

(A) ApoB lipoprotein levels measured by ELISA.

(B) EQ UltraPure removes ~ 96% of ApoB from serum.

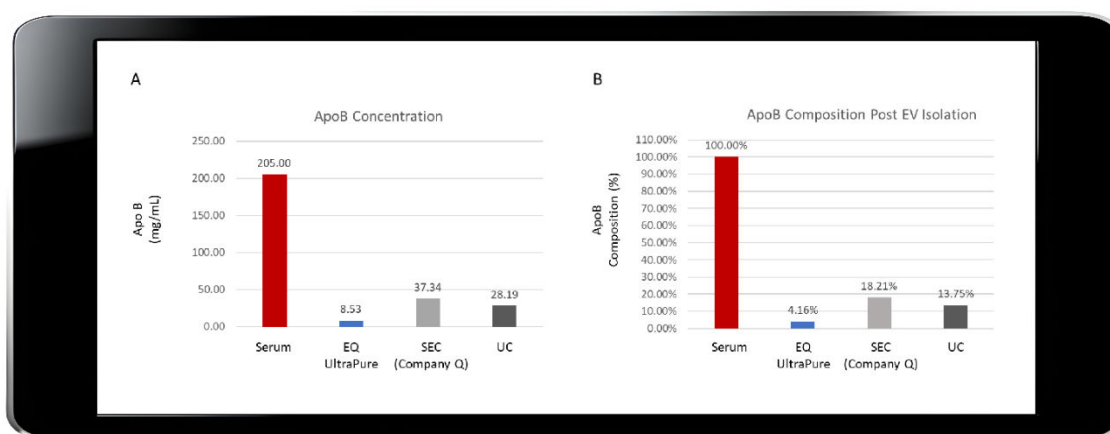


FIGURE 4. EXOQUICK® ULTRAPURE ENABLES EFFICIENT LIPOPROTEIN REMOVAL.

High-Quality EV RNA, Every Time.

EV RNA isolated with EQ UltraPure and the EVery EV RNA Kit (Cat# Every100B-1) shows high quality by Agilent Bioanalyzer electropherogram and gel analysis (Figure 5).

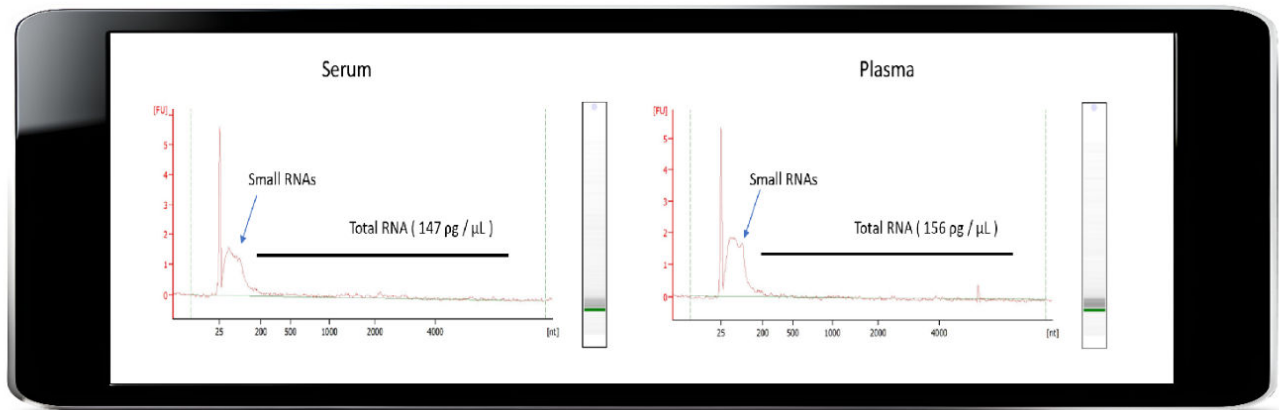


FIGURE 5. EV RNA QUALITY ASSESSMENT BY BIOANALYZER.

TECHNICAL SUPPORT

For more information about SBI products and to download manuals in PDF format, please visit our web site:
<http://www.systembio.com>

For additional information or technical assistance, please call or email us at:

System Biosciences (SBI)
2438 Embarcadero Way
Palo Alto, CA 94303

Phone: (650) 968-2200
Toll-Free: (888) 266-5066
Fax (650) 968-2277

E-mail:
General Information: info@systembio.com
Technical Support: tech@systembio.com
Ordering Information: orders@systembio.com

LICENSING AND WARRANTY STATEMENT

Limited Use License

Use of SmartSEC-TC for EV Isolation (*i.e.*, the “Product”) is subject to the following terms and conditions. If the terms and conditions are not acceptable, return all components of the Product to System Biosciences (SBI) within 7 calendar days. Purchase and use of any part of the Product constitutes acceptance of the following terms.

- The purchaser of the Product is granted a limited license to use the Product under the following terms and conditions:
- The Product shall be used by the purchaser for internal research purposes only. The Product is expressly not designed, intended, or warranted for use in humans or for therapeutic or diagnostic use.
- The Product may not be resold, modified for resale, or used to manufacture commercial products without prior written consent of SBI.

This Product should be used in accordance with the NIH guidelines developed for recombinant DNA and genetic research.

This Product is covered by licensed Patents. For information concerning licenses for commercial use, contact SBI.

Purchase of the product does not grant any rights or license for use other than those explicitly listed in this Licensing and Warranty Statement. Use of the Product for any use other than described expressly herein may be covered by patents or subject to rights other than those mentioned. SBI disclaims any and all responsibility for injury or damage which may be caused by the failure of the buyer or any other person to use the Product in accordance with the terms and conditions outlined herein.

Limited Warranty

SBI warrants that the Product meets the specifications described in this manual. If it is proven to the satisfaction of SBI that the Product fails to meet these specifications, SBI will replace the Product or provide the purchaser with a refund at SBI's sole discretion. This limited warranty shall not extend to anyone other than the original purchaser of the Product. Notice of nonconforming products must be made to SBI within 30 days of receipt of the Product.

SBI's liability is expressly limited to replacement of Product or a refund limited to the actual purchase price. SBI's liability does not extend to any damages arising from use or improper use of the Product, or losses associated with the use of additional materials or reagents. This limited warranty is the sole and exclusive warranty. SBI does not provide any other warranties of any kind, expressed or implied, including the merchantability or fitness of the Product for a particular purpose.

SBI is committed to providing our customers with high-quality products. If you should have any questions or concerns about any SBI products, please contact us at (888) 266-5066.

© 2025 System Biosciences (SBI), All Rights Reserved

THIS PAGE LEFT INTENTIONALY BLANK

THIS PAGE LEFT INTENTIONALLY BLANK

SYSTEM BIOSCIENCES, LLC

2438 Embarcadero Way
Palo Alto, CA 94303

info@systembio.com
systembio.com

Toll free: (888) 266-5066



System
Biosciences



FUELING YOUR INNOVATION

